### $\begin{array}{c} \textbf{Masimo Sensors} \\ \textbf{RD SET}^{\text{TM}} \end{array}$

Featuring Masimo SET<sup>®</sup> Measure-through Motion and Low Perfusion<sup>™</sup> Technology



- > Maximising Patient Comfort
- > Optimising Clinician Workflow
- > Helping Hospitals Meet Their Green Initiatives 😂



### **RD SET Sensors for Patients** MAXIMISING > FLAT SENSOR CABLE PATIENT COMFORT > Flat, lightweight sensor cable with smooth edges lies comfortably on the patient's hand or foot Lightweight sensor with a flat, soft cable > LIGHTWEIGHT CONNECTOR > Made from materials that result in a lightweight connector with no moving parts > SMALL, THIN OPTICAL COMPONENTS > Low profile internal components allow the sensor to better conform to the shape of a finger and may put less pressure on the measurement site > Orientation of optical components position the sensor cable comfortably on top of the hand

#### **RD SET Sensors for Caregivers**

# OPTIMISING CLINICIAN WORKFLOW

Simple to use with enhanced connection and sensor application features for a better user experience

#### > TWO STYLES OF SENSORS FOR USE ON DIFFERENT PATIENT TYPES




#### Wrap-around Style Sensors

- > Available in adult, paediatric, infant, and neonatal sizes
- > Easily removed and reapplied
- > Suited for patients with long fingernails or finger deformities



**SpO2** accuracy has improved in conditions of motion and no motion, providing clinicians with greater confidence when monitoring oxygenation status.



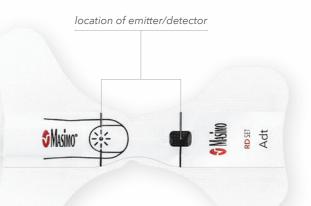



#### Fold-over Style Sensors

- > Available in adult and paediatric sizes
- > Offering a more secure application to the digit and more intuitive sensor alignment





PROPER SENSOR APPLICATION


- > Application graphics printed on top and bottom of sensors to assist with sensor application for optimal performance and ease of sensor removal and reapplication
- Sensor labels to immediately communicate location of emitter/detector



#### **RD SET Sensors for the Environment**

## HELPING HOSPITALS MEET THEIR GREEN INITIATIVES

The same Masimo SET® performance with a significant reduction in waste

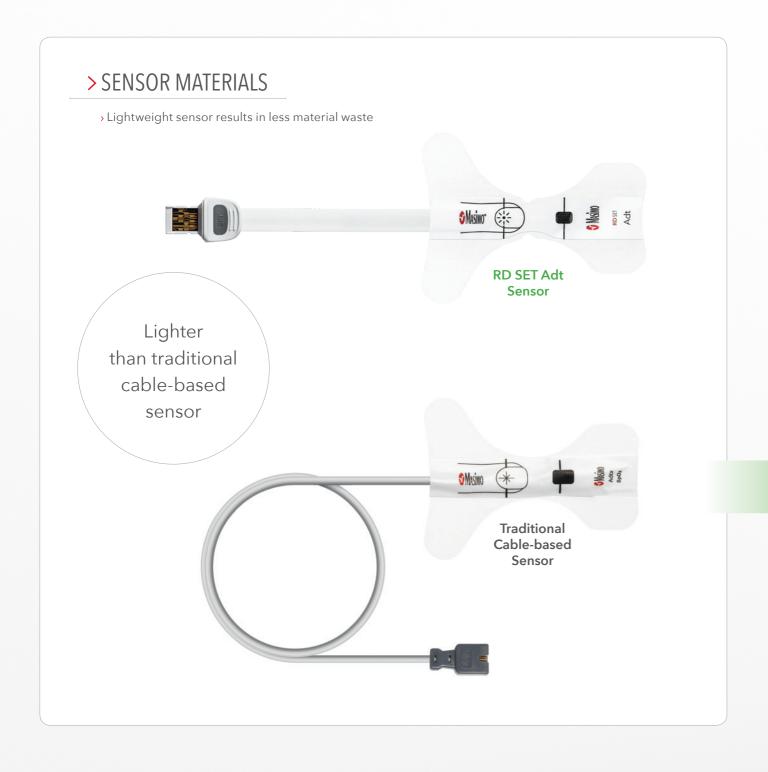

#### > PACKAGING DESIGN

- > RD SET sensors utilise significantly smaller packaging
- Lightweight package design is easy to handle

Sleek recyclable packaging reduces storage space by 44%\* Volume: 181.25 inches³ (460.375 cm³)

Traditional Cablebased Sensor Box Box of 20

Volume: 100.48 inches³ (255.22 cm³)



RD SET Sensor Box Box of 20

Storage space reduction calculated by dividing the reduction in volume by volume of the traditional cable-based sensor box.

> LIGHTWEIGHT SENSOR AND PACKAGING DESIGN FOR A GREEN SOLUTION



Traditional Cablebased Sensors

Up to 84% less
waste with Adult RD
SET sensors versus
traditional cablebased sensors\*\*



RD SET Sensors

\*\*Waste calculated by comparing the sensor and packaging weight of traditional cable-based sensors versus Adult RD adhesive sensors. Internal data on file

#### **APPLICATION**



RD SET Adt finger application



RD SET Pdt finger application



RD SET Inf thumb application



RD SET Neo foot application



RD SET NeoPt / NeoPt-500 foot application

#### **DISPOSABLE SENSORS**







Masimo's Soffouch line of sensors is designed to be used whenever skin sensitivity issues are a concern, such as with extremely low birth weight infants. Masimo Soffouch sensors incorporate soft foam and VelAid hook and loop attachment wraps that come in a variety of configurations to address a wide range of clinical uses.

#### RD SET DISPOSABLE SENSOR SERIES SPECIFICATIONS

ACCURACY – (A <sub>RMS</sub> ) <sup>1,2</sup>	
RD SET Sensors (Adt, Pdt, Inf, Neo) >3kg  SpO2 Accuracy Range.  No Motion  Motion  Low Perfusion.	
PR Accuracy No Motion  Motion Low Perfusion	5 bpm
RD SET Sensors (Neo, NeoPt, NeoPt-500) < 3kg SpO2 Accuracy Range. No Motion Motion. Low Perfusion.	
PR Accuracy No Motion Motion Low Perfusion	5 bpm
Sp02 Limits of Agreement (LoA)           Upper 95% LoA (no motion)            Lower 95% LoA (no motion)            Upper 95% LoA (motion)            Lower 95% LoA (motion)	2.3% 2.9%

WEIGHT RANGE	
RD SET Pdt RD SET Inf RD SET Neo (neonatal) RD SET Neo (adult) RD SET NeoPt	>30 kg, finger or toe application 10–50 kg, finger or toe application 3–20 kg, thumb or great toe application <3 kg, hand or foot application >40 kg, finger or toe application <1 kg, hand or foot application <1 kg, hand or foot application
COMPATIBILITY	
Compatible Oximeters	Systems containing Masimo SET® or licensed to use RD SET Series sensors²
INFORMATION	
Single-patient-use / Non-sterile / Packaged 20 per box / Does not contain natural rubber latex	
ORDERING INFORMATION	
	Part Number

RD SET Disposable Sensor Series	Part Number
RD SET Adt	4000
RD SET Pdt	4001
RD SET Inf	
RD SET Neo	
RD SET NeoPt	4004
RD SET NeoPt-500.	4005
RD SET Replacement Tapes/Wraps	Part Number
Replacement Tapes, Inf	4046
Replacement Tapes, Neo	4047
Replacement Wraps, NeoPt	4048
Replacement Wraps, NeoPt-500	4049

<sup>&</sup>lt;sup>1</sup> ARMS accuracy is a statistical calculation of the difference between device measurements and reference measurements. Approximately two-thirds of the device measurements fell within ± ARMS of the reference measurements in a controlled study. <sup>2</sup> Improved accuracy specifications available where cleared, refer to Directions for Use. <sup>3</sup> Accuracy specifications provided reflect use with the following Masimo technology boards and software versions and higher: MS-2000 SB version V5.1, MSX-1 version V5.3, MX-5 version V7.12

For professional use. See instructions for use for full prescribing information, including indications, contraindications, warnings, and precautions.





